


ATTACH WITH APPROPRIATE ADHESIVE TWELVE PLACES

FIELD CAGE I.D. OVERLAPS GAS OUTLET

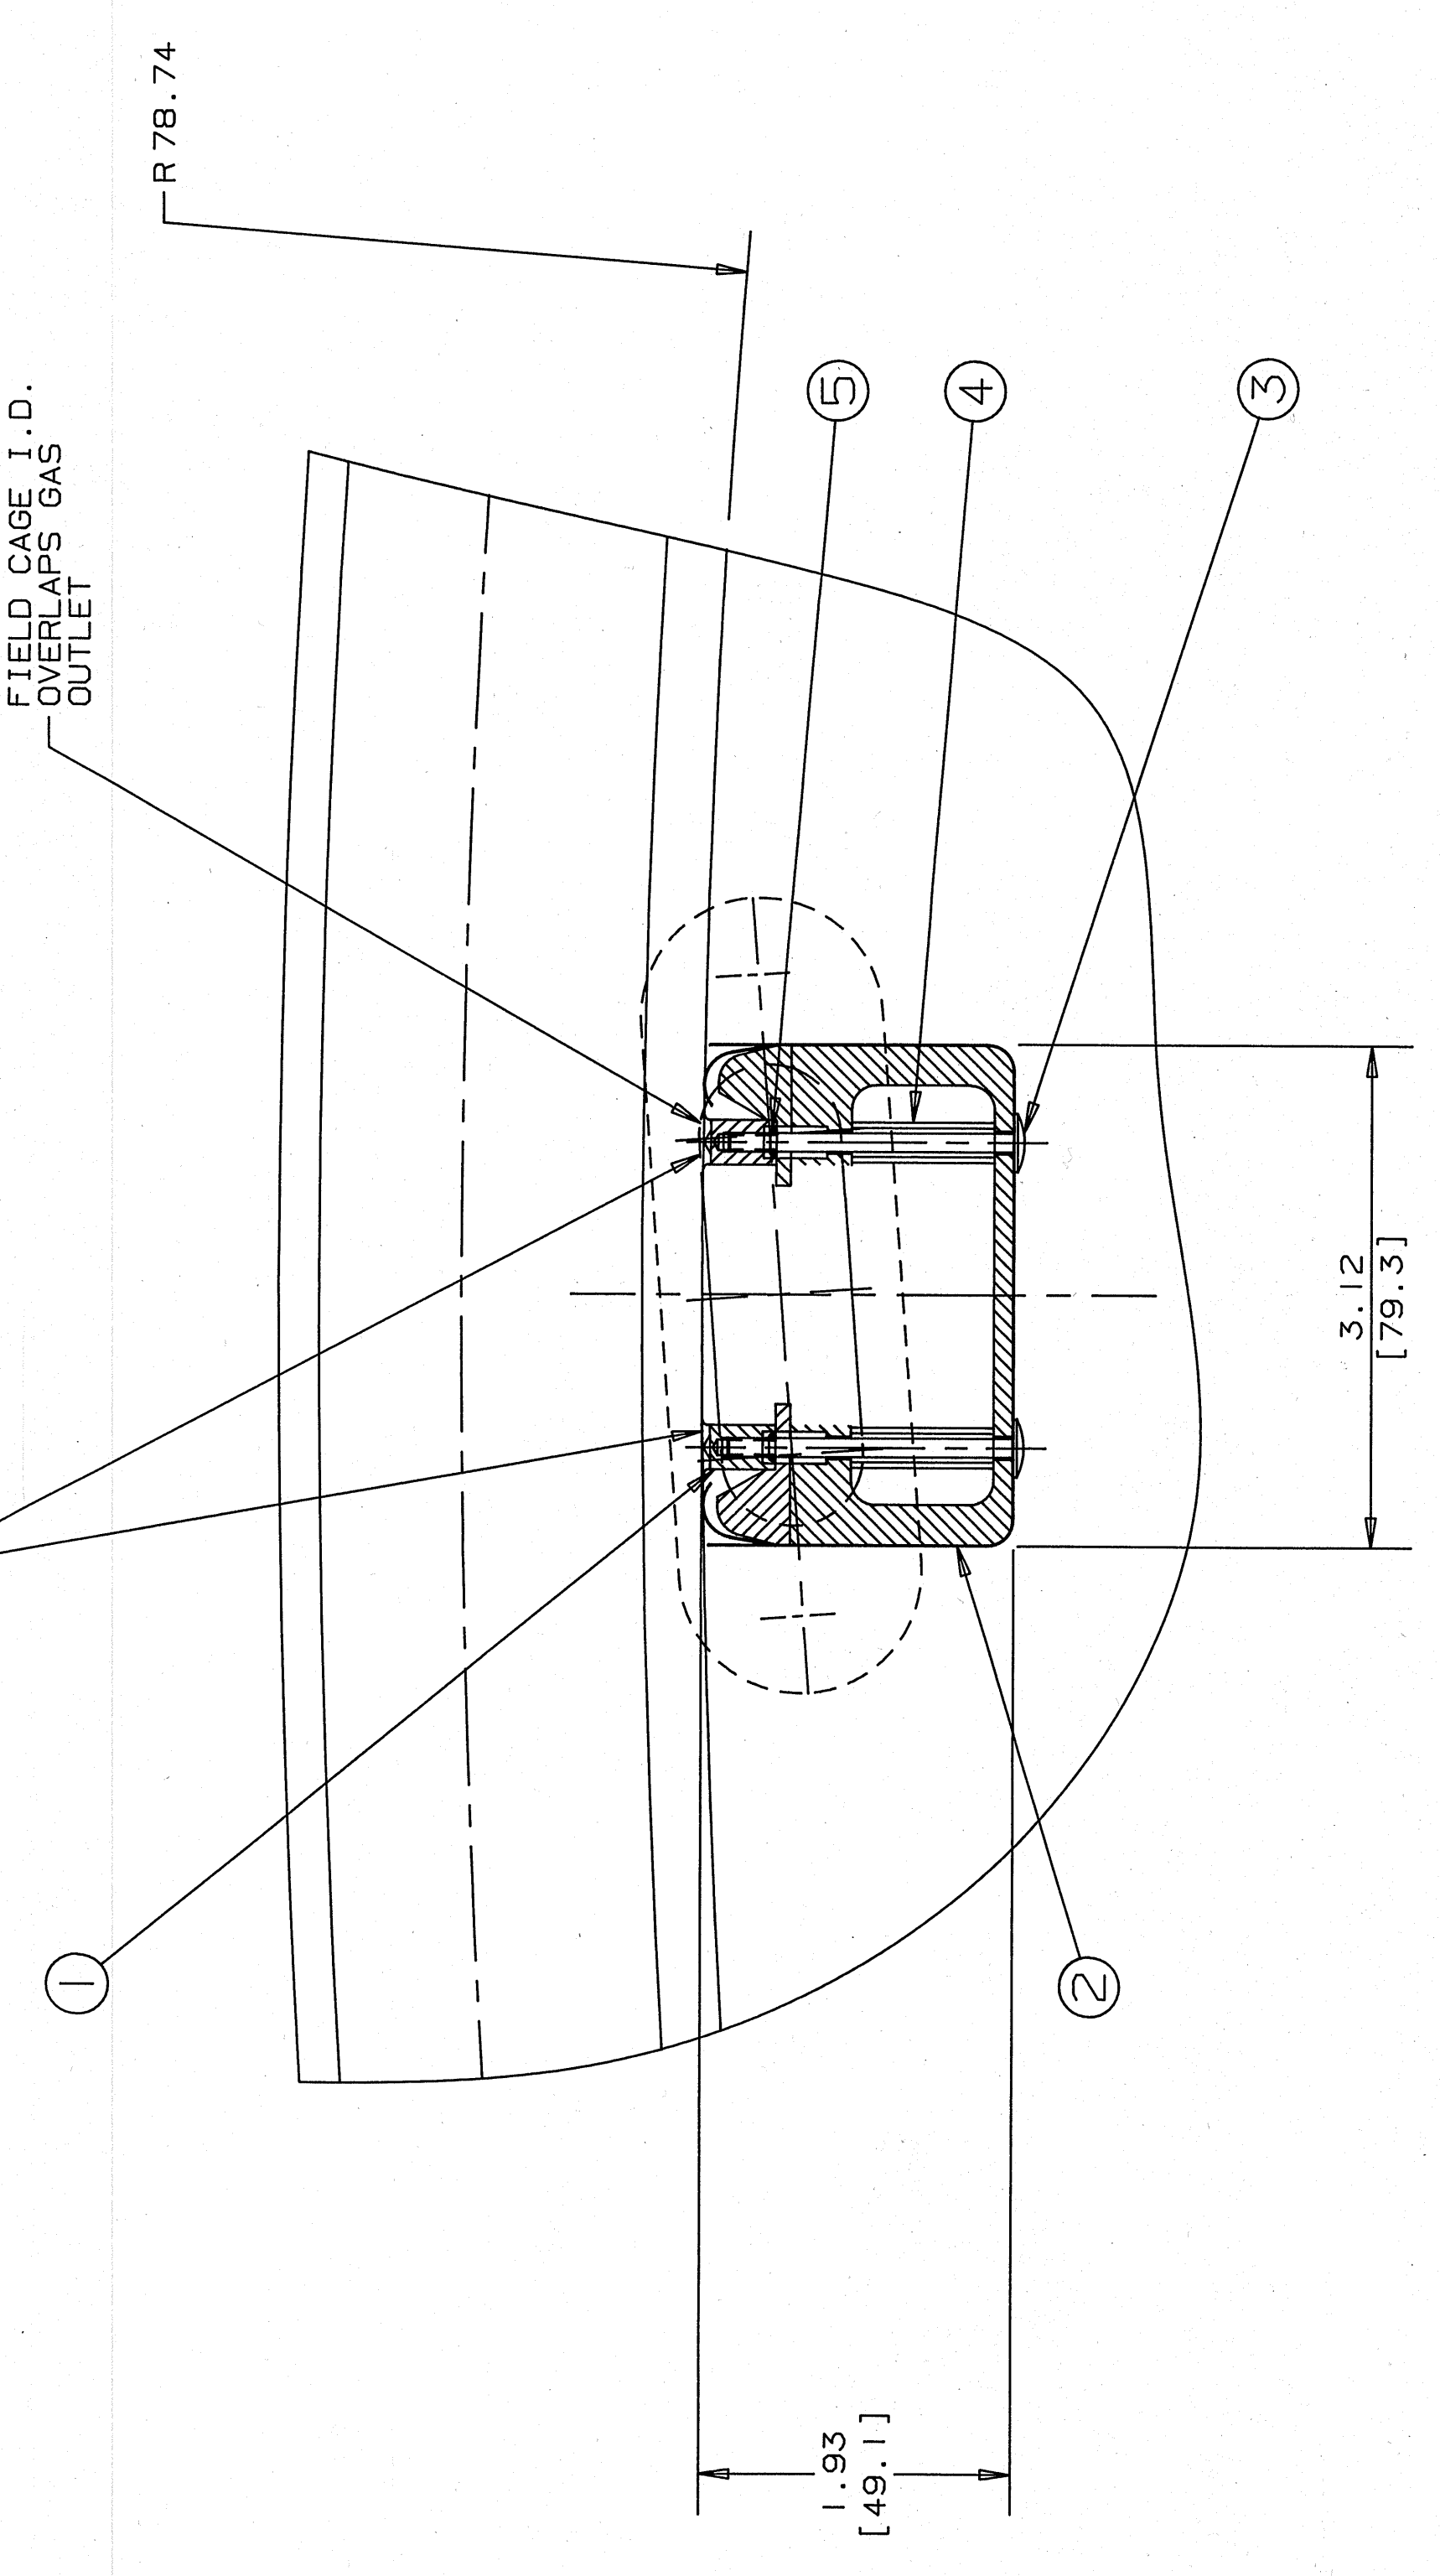

NOTES:

1. VITON O-RINGS MUST BE BOILED IN A DEIONIZED WATER.

SECTION A-A  
 SCALE: FULL

ITEM #	PART NUMBER	DESCRIPTION	QTY	UNIT	REV.	DATE
5	12	O-RING 1/16 I.D. X 1/32 O.S. MINNESOTA RUBBER #8103, VITON (NOTED)				
4	12	RESISTOR COVER SCREW SLERVE				
3	12	RESISTOR COVER MOUNTING SCREW				
2	1	RESISTOR COVER				
1	12	BPT COVER MOUNTING TAB				

REV.	BY	DATE	DESCRIPTION
A	JJA	05/14/96	INITIAL RELEASE
B	JJA	05/20/96	ITEM QUANTITIES 12 WAS 8

REV.	BY	DATE	DESCRIPTION
A	JJA	05/14/96	INITIAL RELEASE
B	JJA	05/20/96	ITEM QUANTITIES 12 WAS 8

REV.	BY	DATE	DESCRIPTION
A	JJA	05/14/96	INITIAL RELEASE
B	JJA	05/20/96	ITEM QUANTITIES 12 WAS 8

REV.	BY	DATE	DESCRIPTION
A	JJA	05/14/96	INITIAL RELEASE
B	JJA	05/20/96	ITEM QUANTITIES 12 WAS 8